

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning documents *will not* correct images,  
please do not report the images to the  
Image Problem Mailbox.**



6702  
A-101-17  
CWL

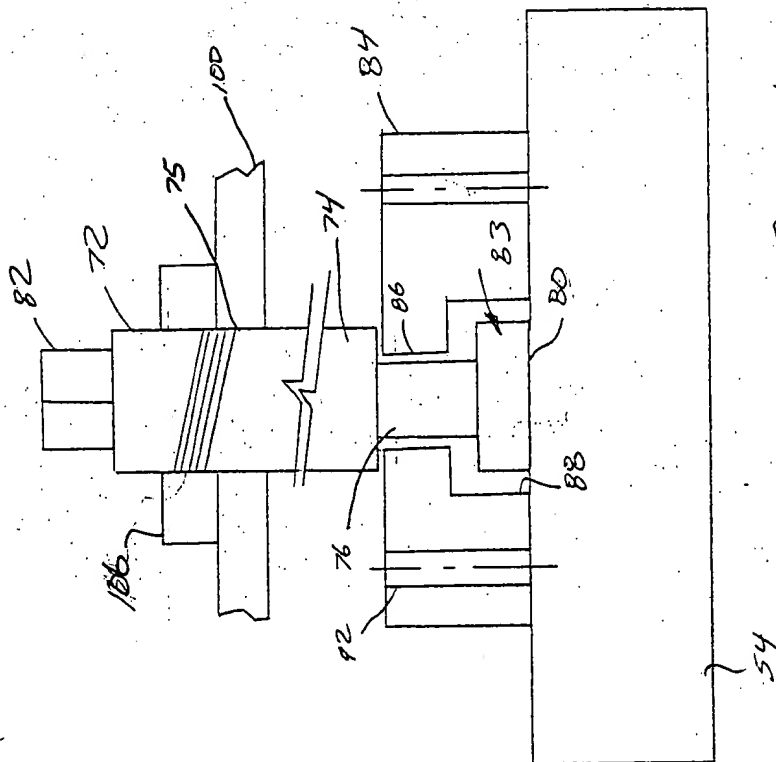


FIG. 3

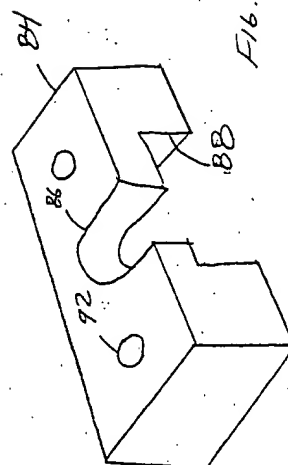


FIG. 4

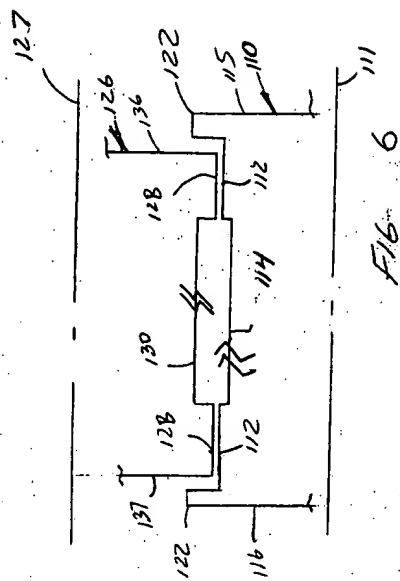


FIG. 6

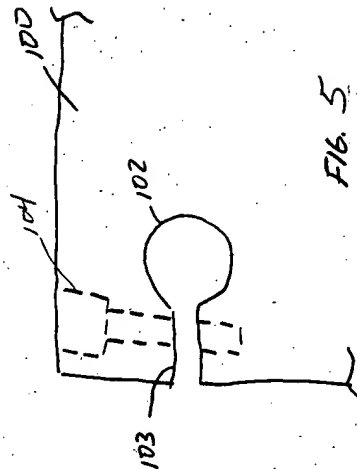


FIG. 5



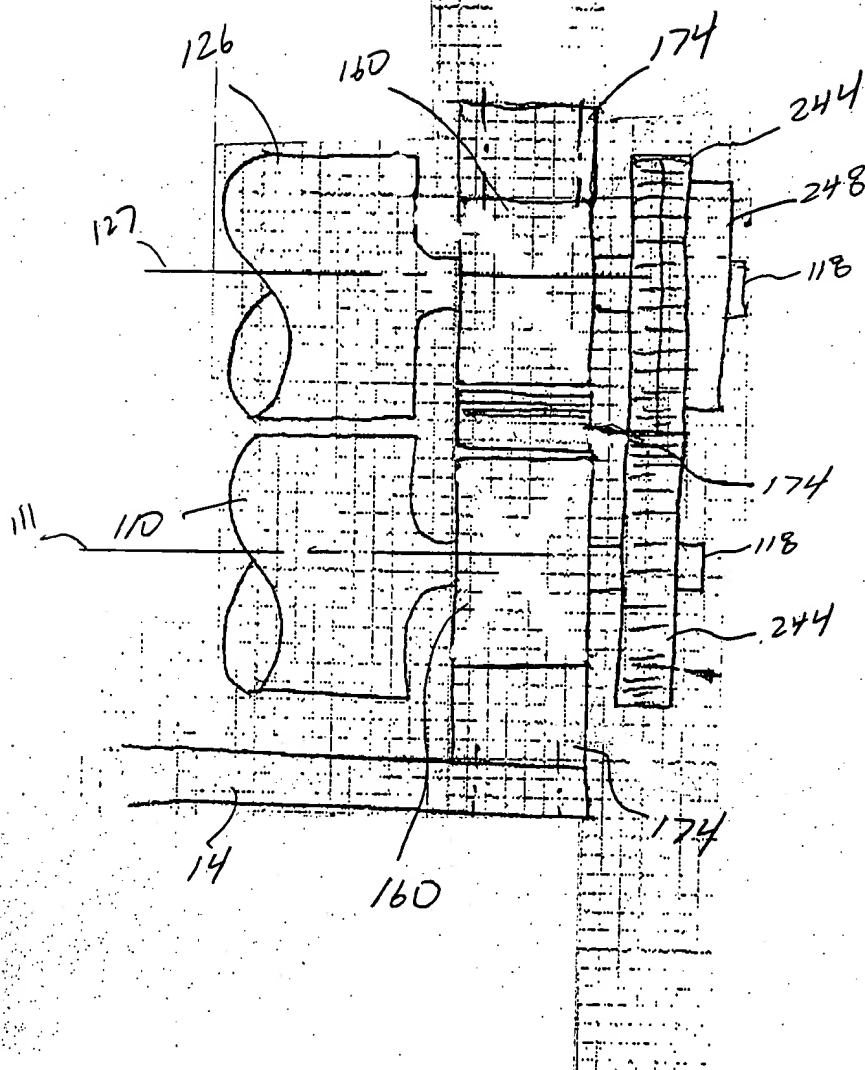


FIG. 8

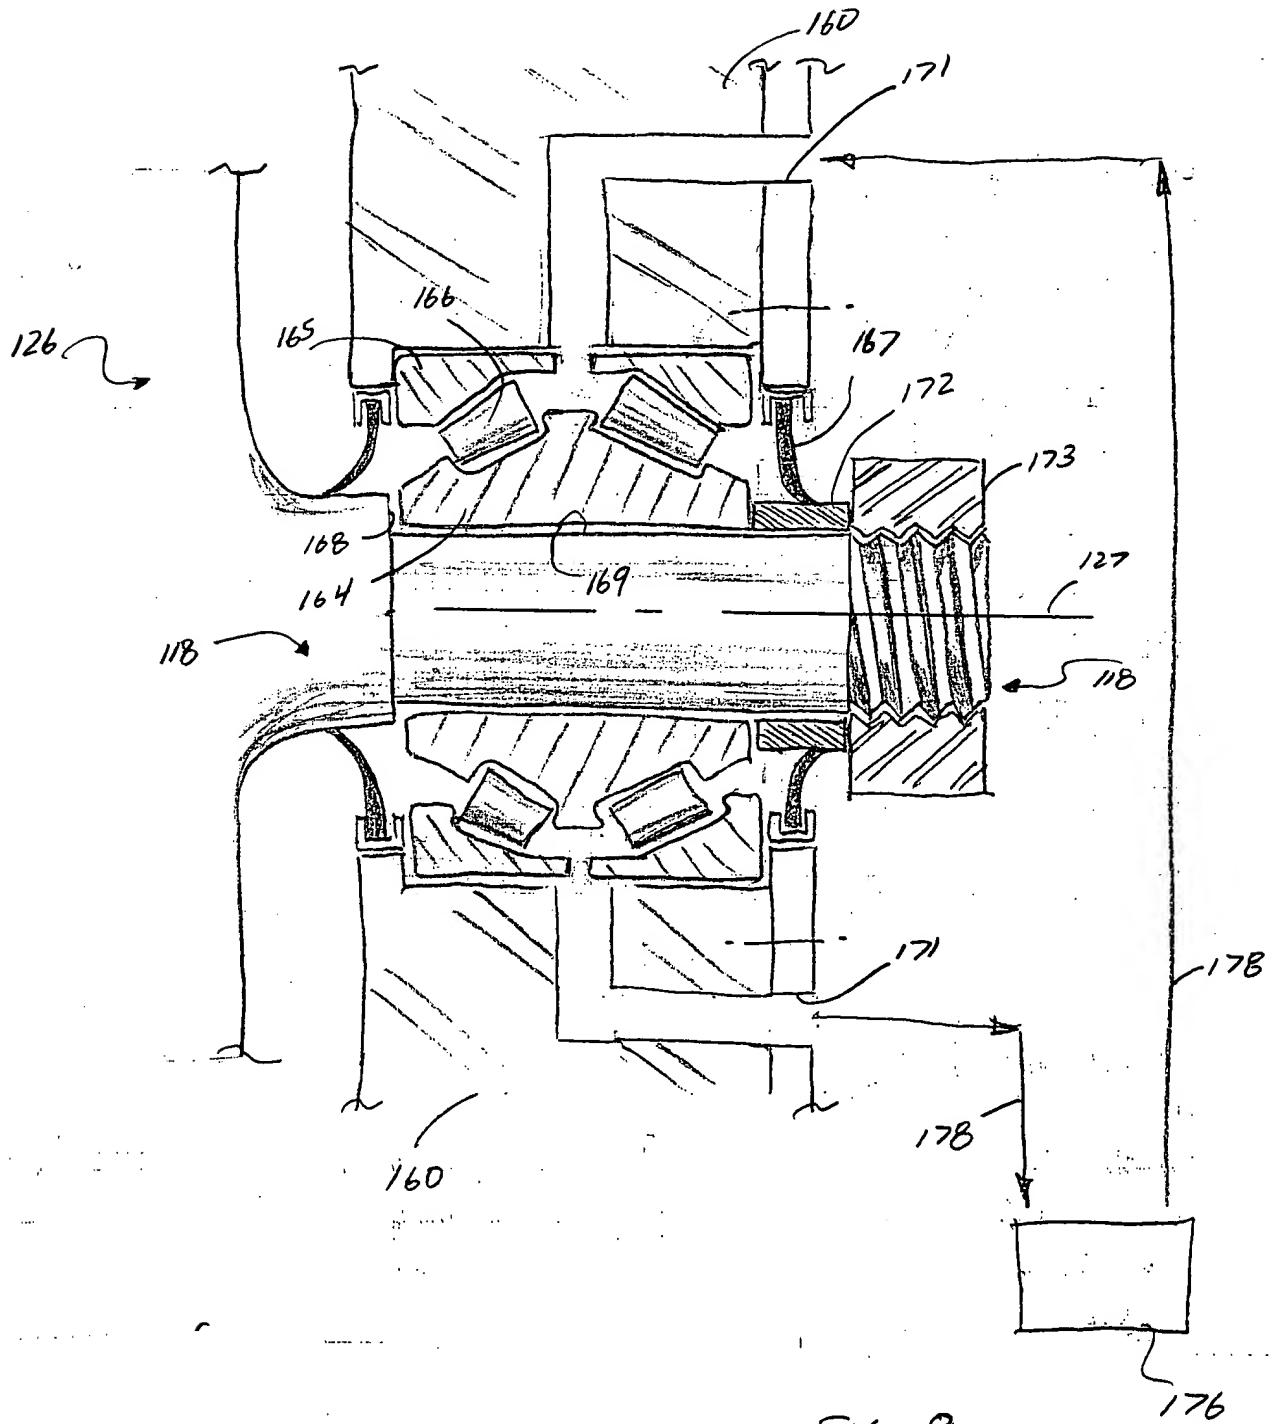


FIG. 9

CWLIDIA  
6 OF 9

FIG. 1 is a perspective view of the device 10, showing the main frame 12, the central cylindrical component 12, and the base 110. The device includes various adjustment mechanisms and structural elements, such as the support structure 106, the base 110, and the adjustment mechanism 116. A warning label is visible on the front of the central component 12, indicating that the device is not to be used for medical purposes. The device is shown in a perspective view, highlighting its three-dimensional structure and the various components that make up the assembly.

7 OF 9

CWL 101 - A



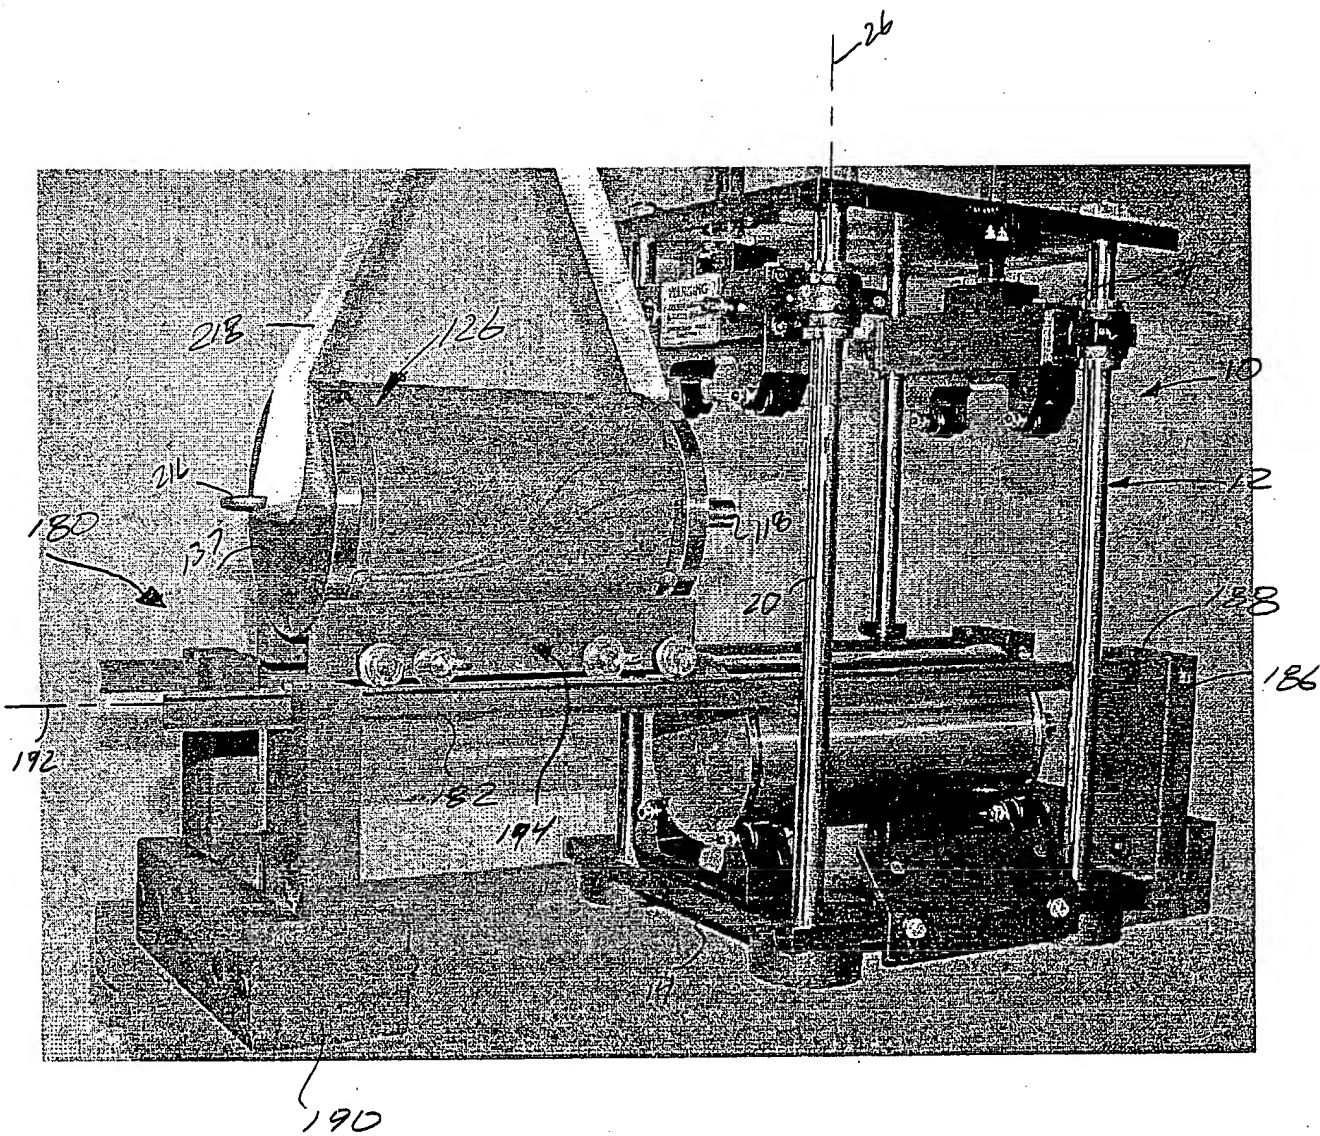


FIG. 11

80F9

CWL100-A

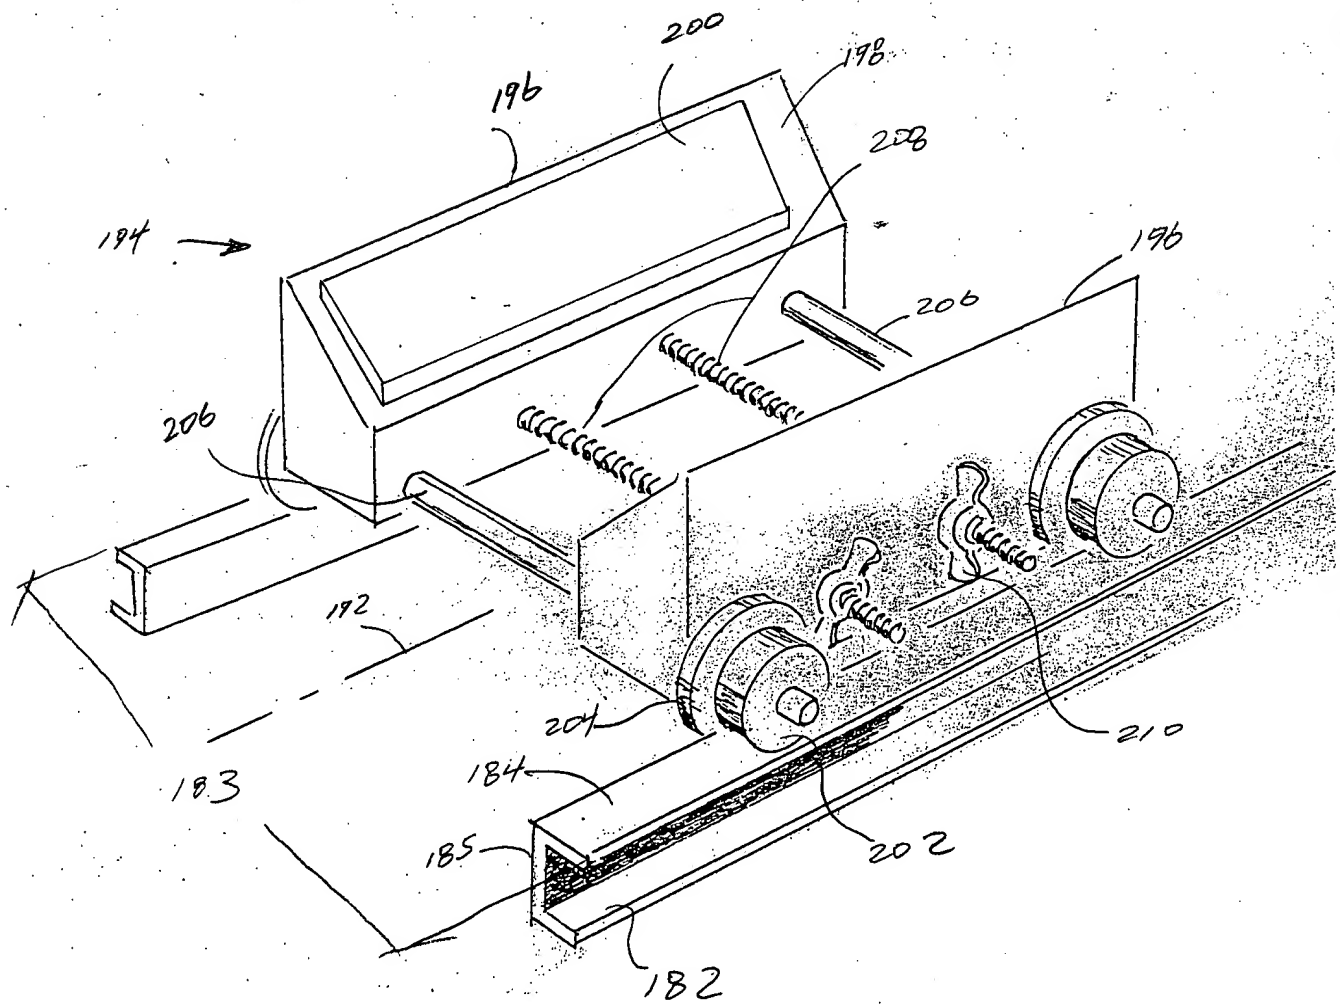


Fig 12

9 OF 9

CWL 101 -A